


Clinical Laboratory Test Update

Effective 11/6/2025, the HOLOGIC Aptima® Unisex Swab Specimen Collection Kit (white label, blue swab) used for Chlamydia trachomatis (CT), Neisseria gonorrhoeae (NG), and Trichomonas amplified RNA testing will be gradually phasing out and being replaced with the Aptima® Multitest Swab (orange label, pink swab).

The Aptima® Multitest Swab (orange label, pink swab) is validated for specimen collection from genital, throat, rectal, and eye sources.

Note: Chlamydia trachomatis and Neisseria gonorrhoeae RECTAL and THROAT **SELF COLLECT** specimens must be collected using the Aptima® Multitest Swab (orange label, pink swab) IMMEDIATELY.

Urine specimens will continue to be collected using the HOLOGIC Aptima® Urine Specimen Collection Kit.

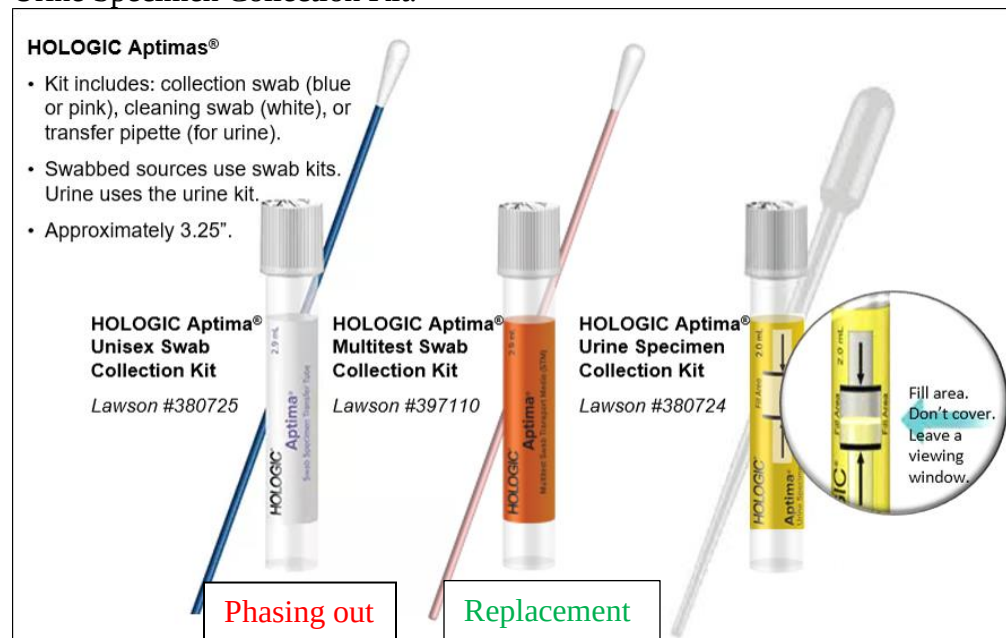

Please call the UCHealth Memorial Hospital Sendout Department at 719.365.2626 if you have any questions.